

OBS-3 AMCO Clear Calibration Certificate

Serial Number: 1591


NTU Range: 250 NTU

Customer: SeaBird Electronics

Output: 0-5000mv

Coefficients

$$y = 6.339E-11x^2 + 4.997E-02x + 1.707E-01$$

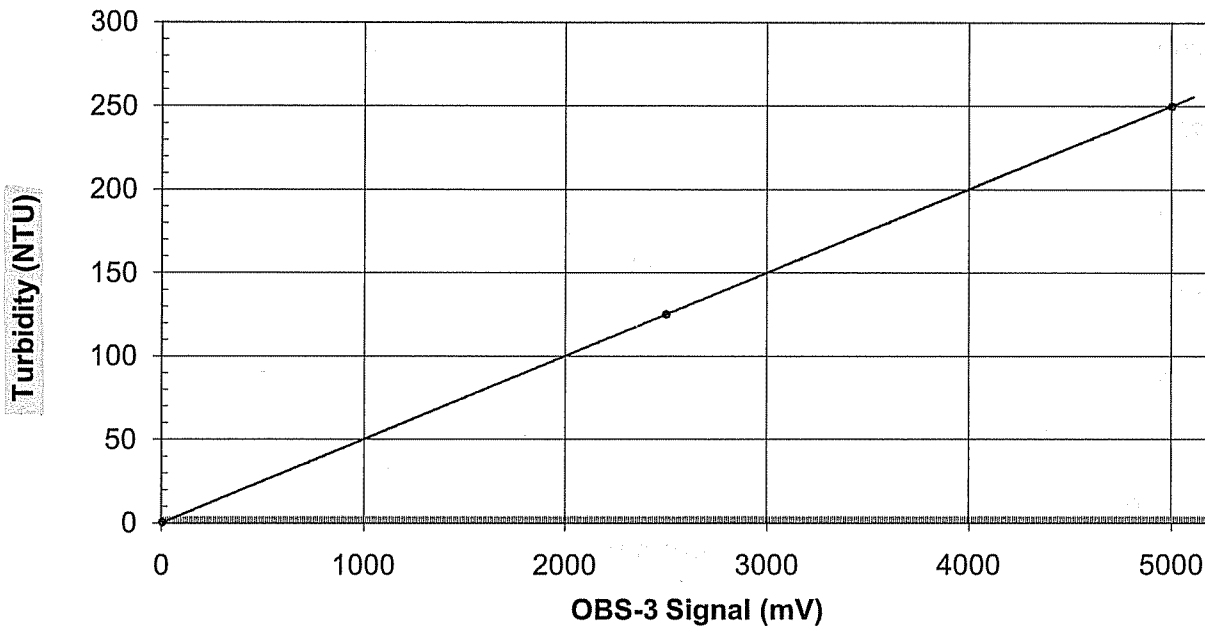

Performed by:



OBS-3 AMCO Clear Calibration Certificate

Serial Number: 1591


NTU Range: 250 NTU

Customer: SeaBird Electronics

Output: 0-5V

Coefficients

$$y = 6.339E-05x^2 + 4.997E+01x + 1.707E-01$$

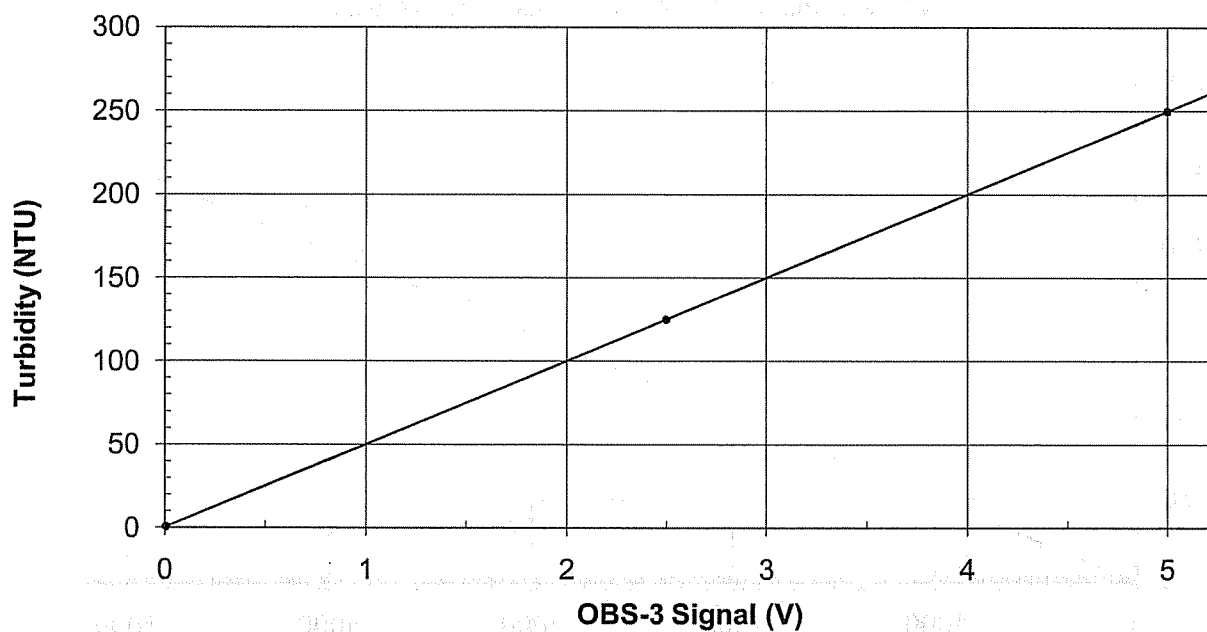

Performed by:



**CAMPBELL®
SCIENTIFIC**